

Certificate of Analysis


Date:	2025-06-04 15:14:34 -04:00	Cultivar:	
Serial:	LL030645	Moisture:	0.0%
LightLab	BW-LABS	Col Tests Remaining:	24
Operator:	DAIANA	CoA Revision:	1
Sample ID:		Calibration Exp:	2026-03-21
Method:	LightLab HPLC	Product:	1000mg Broad Spectrum CBD Tincture
Test Type:	Tinctures (%weight)	SKU:	
Weight / Volume:	0.469 g	Batch:	BT10574
Solvent:	20 ml		
Temperature:	27.3 °C		
Notes:			
SA Botanicals 11255 Huebner Rd. #101 San Antonio, TX 78230			

Cannabinoid Profile

Analyte	Per 30.000 g Serving (mg)	Per 1.0 Pieces(mg)	%	LOQ
THC-A	ND	ND	ND	0.21
Δ9-THC	ND	ND	ND	0.21
CBD-A	ND	ND	ND	0.21
CBG-A	ND	ND	ND	0.21
CBD/CBG	914.3	914.3	3.0	0.21
CBN-A	ND	ND	ND	0.21
CBN	ND	ND	ND	0.21
CBC-A	ND	ND	ND	0.21
CBC	ND	ND	ND	0.21
Δ8-THC*	ND	ND	ND	1.7
Δ10-THC	ND	ND	ND	0.21
THCV-A	ND	ND	ND	0.21
THCV	ND	ND	ND	0.21
Terpenes			ND	
Total THC	ND	ND	ND	
Total Cannabinoids	914.3	914.3	3.0	

ND = Not Detected; n/a = Not Analyzed; LOQ = Limit of Quantification; Total THC = (0.877 x THC-A) + Δ9-THC; Total CBD = (0.877 x CBD-A) + CBD. * Δ8THC has lower precision and higher detection limit than other cannabinoids.

Chromatogram

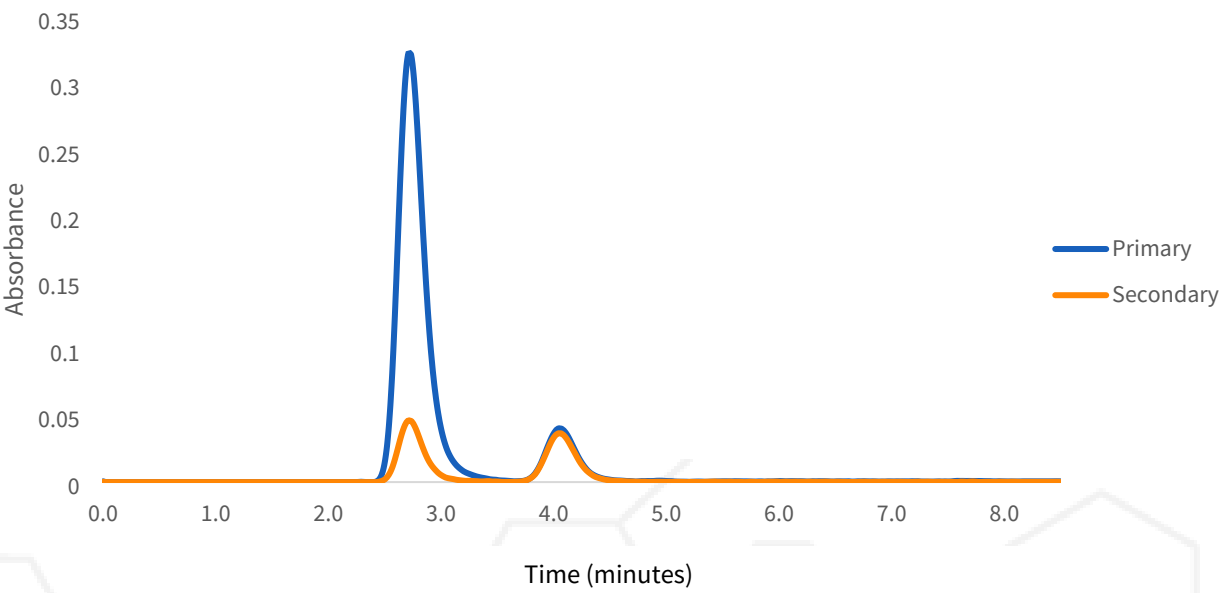

Sample Images



Change History

Date	User	Action
2025-06-04 15:14:34 -04:00		Test Recorded
2025-06-04 15:29:46 -04:00	DA	Changed Operator from "" to "DAIANA". Changed EdblProduct from "" to "1000mg Broad Sprectrum CBD Tincture". Changed Batch from "" to "BT10574". Changed Notes from "" to "SA Botanicals 11255 Huebner Rd. #101 San Antonio, TX 78230".
2025-06-04 15:33:15 -04:00	DA	Added an image
2025-06-04 15:34:01 -04:00		Generated a CoA (revision 0)
2025-06-04 15:34:43 -04:00	DA	Changed EdblProduct from "1000mg Broad Sprectrum CBD Tincture" to "1000mg Broad Spectrum CBD Tincture"
2025-06-04 15:34:47 -04:00		Generated a CoA (revision 1)



<u>Daiana Albertus</u>	<u>6/4/2025</u>	Scan for Authenticity
Approved	Date	

The signatory confirms that the Operator has performed the sample preparation according to the LightLab User's Guide. This report is for quality assurance purposes only. These results relate only to the sample included on this report. Orange Photonics makes no claims as to the efficacy, safety, or risks associated with any detected or non-detected level of any compounds reported herein. Orange Photonics makes no claims regarding the adherence to sample preparation guidelines, by the operator, as outlined in the LightLab User's Guide.

